



Uncertainties of stereo-DIC measurements within the range of thermoforming temperatures

Aniket Dastidar, Abderrahmane Ayadi, Marie-France Lacrampe

► To cite this version:

Aniket Dastidar, Abderrahmane Ayadi, Marie-France Lacrampe. Uncertainties of stereo-DIC measurements within the range of thermoforming temperatures. Journée scientifique de la fédération lilloise de mécanique, Sep 2021, Villeneuve d'Ascq, France. hal-04063129

HAL Id: hal-04063129

<https://imt-nord-europe.hal.science/hal-04063129>

Submitted on 8 Apr 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/358147471>

Uncertainties of stereo-DIC measurements within the range of thermoforming temperatures

Poster · September 2021

CITATIONS

0

READS

6

3 authors:



Aniket Ghosh Dastidar

IMT Lille Douai

6 PUBLICATIONS 1 CITATION

[SEE PROFILE](#)



Abderrahmane AYADI

IMT Nord Europe

33 PUBLICATIONS 246 CITATIONS

[SEE PROFILE](#)



Marie France Lacrampe

IMT Lille Douai

149 PUBLICATIONS 3,275 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



Thermoplastic nanocomposites [View project](#)



Hybrid experimental-numerical mechanics applied to thermoforming [View project](#)

Uncertainties of stereo-DIC measurements within the range of thermoforming temperatures

1.CONTEXT

- Stereo-DIC is an optical-numerical technique which can be used for « in-situ » monitoring of materials during the thermoforming processes.
- Within laboratory confines (i.e. under controlled environment), kinematic and deformation full-fields can be measured.

Table.1: Cases that were studied by our research-team:

Experimental studies	Numerical studies
<ul style="list-style-type: none"> Measurement of out-of-plane curvatures and monitoring thinning of thermoplastic sheets [1]. 	<ul style="list-style-type: none"> Implementation of FEMU based inverse identification procedures for material properties [2].

[1] Ayadi. A, Lacrampe MF, P. krawczak. Int. J. Mat. Forming; 13 (2020), 59–76.

[2] Dastidar A.G., Ayadi A. , Lacrampe MF. Procedia Manufacturing, 47 (2020): 933-939.

Authors

- Aniket G. ASTIDAR
- Dr. Abderrahmane AYADI
- Prof. Marie-France LACRAMPE

Department

Centre for Education, Research and Innovation in Materials and Processes (CERI MP).

3.EXPERIMENTAL SETUP

Table.2: Experimental setup details

Setereo-cameras	Camera 1	Camera 2
Positions (mm)	(-14.2, -195.2, 645.8)	(-22.3, -192.4, 653.9)
Rotations (°)	(37.0, -2.9, -2.1)	(36.0, 6.4, -0.8)
Focal length (mm)	43.16	43.34
Pixel size (μm)		5.5
Heating chamber		
Tested temp.	{25, 105, 110, 115, 120}°C	
DIC settings		
Software	DaVis (LaVision)	Software
Subset	19*19	Subset
Stepsize	9*9	Stepsize
Shape function	6 th order spline	Shape function

- Step1:** Re-generation of heat waves in a convective environment within the thermoforming window.

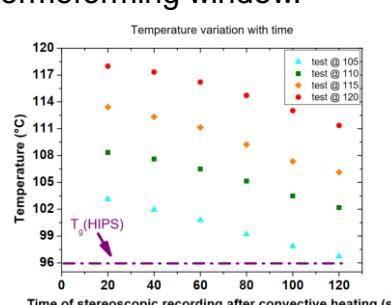
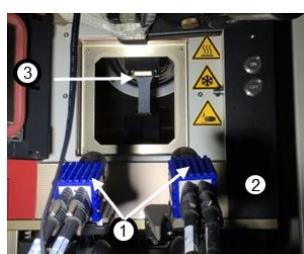


Fig.3: Equipment (left), temperature while recording (right).

4.RIGID BODY TESTS

Step2. Identification of the reference state ($u_y = 0$)

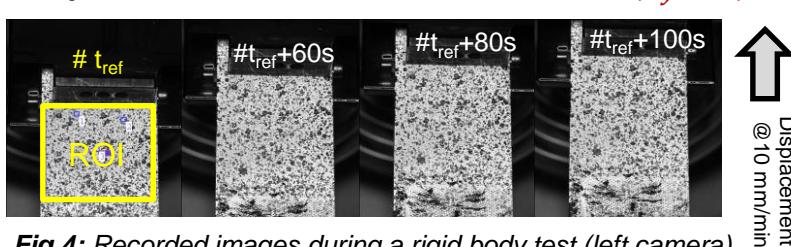


Fig.4: Recorded images during a rigid body test (left camera).

PERSPECTIVES

- More focus will be attributed to initial few seconds of stereoscopic recordings.
- The procedure will be extended to quasi-static stretching tests in the thermoforming range of temperatures.

2.OBJECTIVE

- The current study, sheds light on the accuracy of displacement measurements with the presence of heat waves which affect refractive index homogeneity during thermoforming processes.

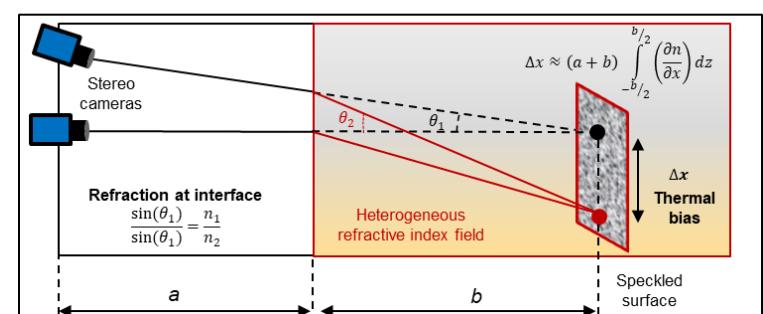


Fig.1: Schematic illustration of the studied problem.

- The main objective** is to evaluate the sensitivity of random and bias errors within the range of thermoforming window of thermoplastics (such as HIPS).

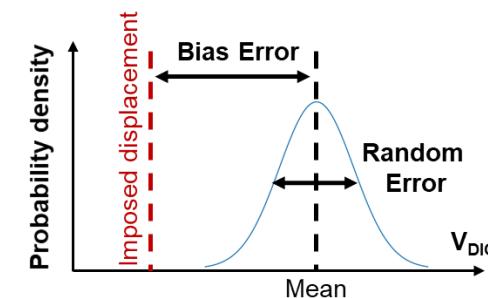


Fig.2: Statistical representation of bias and random errors in the case of a Gaussian distribution.

5.RESULTS

Step 3: DIC computation of disp. vectors (u_y, T)

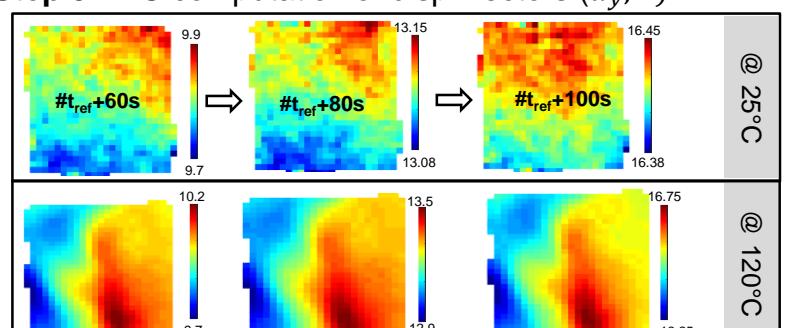


Fig.5: u_y component of stereo-DIC displacement vectors in mm.

Step 4: Evaluation of Random and bias errors

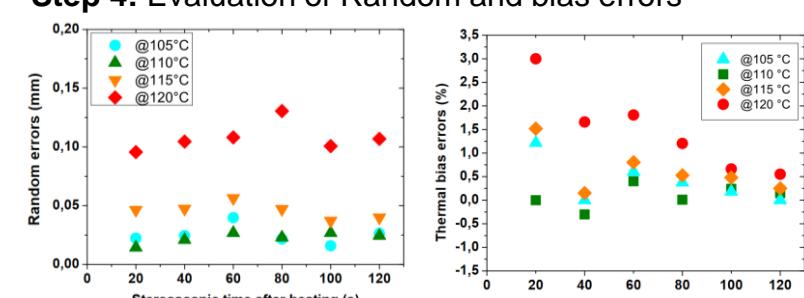


Fig.6: Errors evolution during stereoscopic recording time following convective heating

- Random errors only depend of the identified reference state of the speckled surface after heating.
- Bias errors are sensitive to the heat wave attenuation during stereoscopic recording. Thus, stereo-DIC measurements require temporal filtering of errors.